

DOCUMENTATION

REF. CV-41 / EKN

MASK ULTRA PROTECTION FFP2

MASCARILLA ULTRA PROTECCIÓN FFP2

MASQUE FFP2 ULTRA PROTECTION FFP2

MASCHERINA PROTEZIONE ULTRA FFP2



MASTER BOX: 1000 pcs



CV-41

COLOR: BLANCO/WHITE

ITEM: EKN

DESCRIPTION: NAAMIO

MATERIAL:

5 PLY (46% non woven, 30% Meltblown, 24% algodón).

QUANTITY: 1.000

G.W:

N.W:

CNT SIZE:

BATCH NUMBER:

PRODUCTION DATE:

VALIDITY:


MADE IN P.R.C.

BOX: 25 pcs

L138xW138xH110mm

FFP2
Personal Protective Equipment (PPE)
Equipo de Protección Individual (EPI)


EN 149:2001+A1:2009
FFP2 NR
Filtration Efficiency ≥ 94%



CV-41 MASCARILLA ULTRA PROTECCIÓN FFP2
Comfortable protection against infection / Protección cómoda contra infecciones.

MASCARILLA ULTRA PROTECCIÓN FFP2
Personal Protective Equipment (PPE)
Equipo de Protección Individual (EPI)

Instructions:



Step for usage:

1. Open the foldable mask.
2. Make the nose bridge bar on the up side.
3. Put the strap onto the ear.
4. Adjust the soft bar to fit the nose.
5. Make sure you can breathe well and readjust if necessary.

Instrucciones de uso:

1. Abra la máscara plegable.
2. Ajuste la máscara en la parte superior de la nariz.
3. Ajuste las cintas elásticas por detrás de las orejas.
4. Amoda la pinza nasal a la parte superior de la nariz.
5. Asegúrese de poder respirar bien y ajústelo si es necesario.

Warnings:


1. This mask marked "NR" is for single use only.
2. This mask helps to protect against certain particulate contaminants but does not completely eliminate exposure to the risk of contracting disease or infection.
3. Change the mask immediately if breathing becomes difficult or the mask becomes damaged or distorted.

Atención:

1. Esta máscara "NR" no es recomendada para un solo uso.
2. Esta máscara ayuda a proteger contra ciertas partículas contaminantes, pero no elimina por completo la exposición al riesgo de contraer enfermedades o infecciones.
3. Cambie la máscara inmediatamente si la respiración se vuelve difícil o la máscara se daña o se distorsiona.

FFP2
Personal Protective Equipment (PPE)
Equipo de Protección Individual (EPI)

EN 149:2001+A1:2009
FFP2 NR
Filtration Efficiency ≥ 94%



CV-41 MASCARILLA ULTRA PROTECCIÓN FFP2
Comfortable protection against infection / Protección cómoda contra infecciones.

Regulation/Regulation: 2016/425
FFP2
Equipo de Protección Individual (EPI)
Personal Protective Equipment (PPE)
Model: EKN

CE 0598
EN 149:2001+A1:2009
FFP2 NR
Filtration Efficiency ≥ 94%

Importado por / Imported by:
B30668420, C/ Sofia, 3-5
Pol.Ind. Cabezo Beaza 30353 Cartagena (Spain)

Organismo notificado / Notified body:
SGS FRANK OY
Täskentienkatu 8, FI-00380 Helsinki, Finland

FABRICANTE / MANUFACTURER:
CHANGTING TRANGLE SANITARY ARTICLES CO.,LTD
ASEL Middle Changting Street Economic
Development Zone, Longyan City, Fujian Province, China
MADE IN P.R.C.

Cantidad por caja 25 Piezas
Quantity per box 25 Pieces

Comprobación certificados/
Certificate verification:
www.certificados.cifra.es

BAG: 1 pc 133x133 mm

Regulación/Regulation: 2016/425

FFP2

MASCARILLA ULTRA PROTECCIÓN
ULTRA PROTECTION MASK

Equipo de Protección Individual (EPI)
Personal Protective Equipment (PPE)

Model: EKN



CE 0598
EN 149:2001+A1:2009
FFP2 NR
Filtration Efficiency ≥ 94%


Importado por / Imported by:
B30668420, C/ Sofia, 3-5
Pol.Ind. Cabezo Beaza 30353 Cartagena (Spain)

Organismo notificado / Notified body:
SGS FRANK OY
Täskentienkatu 8, FI-00380 Helsinki, Finland

FABRICANTE / MANUFACTURER:
CHANGTING TRANGLE SANITARY ARTICLES CO.,LTD
ASEL Middle Changting Street Economic
Development Zone, Longyan City, Fujian Province, China
MADE IN P.R.C.

Cantidad por caja 25 Piezas
Quantity per box 25 Pieces

Comprobación certificados/
Certificate verification:
www.certificados.cifra.es



INSTRUCCIONES DE USO:

1. Abra la máscara plegable.
2. Ajuste la máscara en la parte superior de la nariz.
3. Ajuste las cintas elásticas por detrás de las orejas.
4. Amoda la pinza nasal a la parte superior de la nariz.
5. Asegúrese de poder respirar bien y ajústelo si es necesario.

STEP FOR USAGE:

1. Open the foldable mask.
2. Make the nose bridge bar on the up side.
3. Put the strap onto the ear.
4. Adjust the soft bar to fit the nose.
5. Make sure you can breathe well and readjust if necessary.

ATENCIÓN:


1. Esta máscara "NR" es recomendada para un solo uso.
2. Esta máscara ayuda a proteger contra ciertas partículas contaminantes, pero no elimina por completo la exposición al riesgo de contraer enfermedades o infecciones.
3. Cambie la máscara inmediatamente si la respiración se vuelve difícil o la máscara se daña o se distorsiona.

WARNING:

1. This mask marked "NR" is for single use only.
2. This mask helps to protect against certain particulate contaminants but does not completely eliminate exposure to the risk of contracting disease or infection.
3. Change the mask immediately if breathing becomes difficult or the mask becomes damaged or distorted.

MATERIAL:
46% Non-woven, 30% Meltblown, 24% algodón

MATERIAL:
46% Non-woven, 30% Meltblown, 24% cotton



Fecha de producción / Production date:
Lote / Production Batch:
Plazo de validez / Expiration date:

8 436534 314702



IMPORTANT NOTE:

In all the manufacturing processes of our masks, graphene or its derivatives are not used.

Colaboramos con



Reconocimiento a la responsabilidad ambiental



Universidad Politécnica de Cartagena



UCAM UNIVERSIDAD CATOLICA DE MURCIA

UIMP Cartagena
Universidad Internacional Menéndez Pelayo



Asociaciones y Entidades a las que pertenecemos




EU DECLARATION OF CONFORMITY

Manufacturer: CHANGTING TIANLE SANITARY ARTICLES CO., LTD
Address: Middle Changtingxian Boom Economic Development Zone, Longyan City, Fujian Province, P. R. China

declares that the new PPE described hereafter

Product Name	particle filtering half mask
Model	EKN
Standard	EN 149:2001+A1:2009
Classification	FFP2 NR

Object of the declaration (identification of apparatus allowing traceability. It may include a colour image of sufficient clarity where necessary for the identification of the appearance)

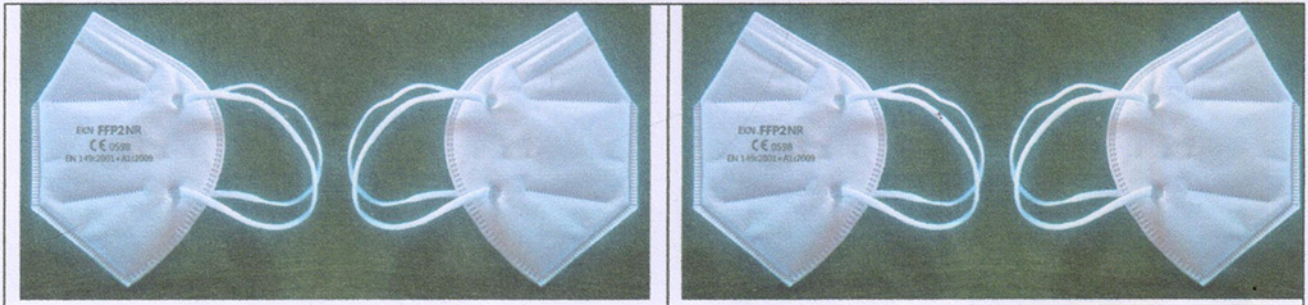

- in conformity with the harmonized standard of EN149:2001+A1:2009.
- performed the EU type-examination (Module B) of the Regulation (EU) 2016/425 and issued the certificate F120/966726
- performed the conformity to type based on internal production control plus supervised product checks at random intervals (module C2) and issued the certificate CN20/42355

Notified Body information

Module B	Module C2
SGS Fimko Oy Takomotie 8, FI-00380 Helsinki, Finland Notified Body No. 0598	SGS Fimko Oy Takomotie 8, FI-00380 Helsinki, Finland Notified Body No. 0598

Signed for of Company

Name: Lin Teng
Position: general manager
Date: 2020. 12. 18
Signature: Lin Teng



CHANGTING TIANLE SANITARY ARTICLES CO.,LTD


Middle Changtingxian Boom Economic Development Zone,
Longyan City, Fujian Province, P.R.China

It is certified that the manufacturer's technical file and the PPE product detailed on
page 2 have been assessed and found to be in accordance with

Regulation (EU) 2016/425 Module B, EU type-examination

This certificate is valid from 29 September 2020 until 29 September 2025
1. Certified since 29 September 2020

Authorised by

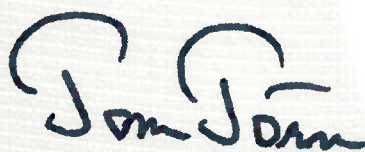


FINAS
Finnish Accreditation Service
S003 (EN ISO/IEC 17065)

SGS FIMKO OY, Notified Body 0598

Takomatie 8, FI-00380, Helsinki, Finland
t +358 9 696 361 f +358 9 692 5474 www.sgs.com

Page 1 of 2



This document is issued by the Company subject to its General Conditions of
Certification Services accessible at www.sgs.com/terms_and_conditions.htm.
Attention is drawn to the limitations of liability, indemnification and jurisdictional
issues established therein. The authenticity of this document may be verified at
<http://www.sgs.com/en/certified-clients-and-products/certified-client-directory>.
Any unauthorized alteration, forgery or falsification of the content or appearance
of this document is unlawful and offenders may be prosecuted to the fullest
extent of the law.

CHANGTING TIANLE SANITARY ARTICLES CO.,LTD

Regulation (EU) 2016/425 Module B, EU type-examination

Issue 1

PPE Product

CTTL (logo) EKN particle filtering half mask, consisting of a white five layer (polypropylene/ polypropylene/ polypropylene / polypropylene / polypropylene) disposable face mask, with nose clip and nylon/spandex ear loop.

It is certified that the manufacturer's technical file and the above mentioned PPE have been assessed and found to meet the applicable Essential Health and Safety Requirements in Annex II of Regulation (EU) 2016/425 Personal Protective Equipment

The following have been applied:

EN 149:2001+A1:2009 (Respiratory protective devices - filtering half masks to protect against particles) device classification: FFP2 NR.

This certificate is issued on the strict condition that appropriate checks on manufactured PPE, as detailed in Article 19 (c) of the Regulation are implemented and maintained while the model is in production

Certification is based on technical file reference:

EKN , dated: 2020/8/17.

SGS Reference Number UK/CRS 241793.

This certificate remains the property of SGS Firko Oy to whom it must be returned on request

Certificate CN20/42355

The management system of

CHANGTING TIANLE SANITARY ARTICLES CO.,LTD

Middle Changtingxian Boom Economic Development Zone,
Longyan City, Fujian Province, P.R. China

has been assessed and certified as meeting the requirements of

Regulation (EU) 2016/425 Module C2

For the following activities

Manufacture of CTTL(logo) EKN particle filtering half mask.
(Note: All products marked CE0598 must have a valid EU type-examination certificate issued under Module B or a valid EC type-examination certificate issued under Article 10 of Directive 89/686/EEC.)

This certificate is valid from 12 October 2020
and remains valid subject to satisfactory surveillance audits.
Issue 1. Certified since 12 October 2020

Authorised by

SGS FIMKO OY, Notified Body 0598

Takomotie 8, FI-00380 Helsinki, Finland
t +358 9 696 361 f +358 9 692 5474 www.sgs.com

FINAS
Finnish Accreditation Service
S003 (EN ISO/IEC 17065)



Test Report **SL52035273306701TX** **Date: July 22, 2020**
CHANGTING TIANLE SANITARY ARTICLES CO.,LTD
MIDDLE CHANGTINGXIAN BOOM ECONOMIC DEVELOPMENT ZONE

Page 1 of 9

**THIS REPORT CANCELS AND SUPERSEDES THE TEST REPORT NO.SL52025269522401TX DATE: 2020-07-07 ISSUED BY SGS (SHANGHAI)
UPDATED CLIENT INFORMATION/ SAMPLE INFORMATION.**


The following sample(s) was/were submitted and identified on behalf of the client as:

- Sample Description : (A)particle filtering half mask
- Style No. : EKN
- Sample Color : (A)WHITE
- Test Performed : Selected test(s) as requested by applicant
- Sample Receiving Date : Jun 03, 2020
- Testing Period : Jun 03, 2020 - Jul 07, 2020
- Test Result(s) : Unless otherwise stated the results shown in this test report refer only to the sample(s) tested, for further details, please refer to the following page(s).

Conclusion:

Sample No.	Recommendation Level
(A)	FFP2 NR

Signed for and on behalf of
SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd Testing Center

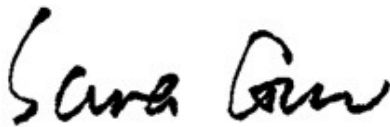

Sara Guo (Account Executive)

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



Test Result

Personal Protective Equipment - Respiratory Protective Devices- Filtering Half Masks to Protect against Particles- Requirements, Testing, Marking

EN 149:2001+A1:2009

Clause 7.4 Packaging

(EN 149:2001+A1:2009 Clause 8.2)

Test Requirement	Results	Comment
Particle filtering half masks shall be offered for sale packaged in such a way that they are protected against mechanical damage and contamination before use.	Comply	Pass

Clause 7.5 Material

(EN 149:2001+A1:2009, Clause 8.2 & 8.3.1 & 8.3.2)

Test Requirement	Results	Comment
Materials used shall be suitable to withstand handling and wear over the period for which the particle filtering half mask is designed to be used.	Comply	Pass
After undergoing the conditioning described in 8.3.1 none of the particle filtering half masks shall have suffered mechanical failure of the facepiece or straps.	Comply	
When conditioned in accordance with 8.3.1 and 8.3.2 the particle filtering half mask shall not collapse.	Comply	
Any material from the filter media released by the air flow through the filter shall not constitute a hazard or nuisance for the wearer.	Comply	

Clause 7.6 Cleaning and Disinfecting

(EN 149:2001+A1:2009, Clause 8.4 & 8.5 & 8.11)

Test Requirement	Results	Comment
If the particle filtering half mask is designed to be re-usable, the materials used shall withstand the cleaning and disinfecting agents and procedures to be specified by the manufacturer. With reference to 7.9.2, after cleaning and disinfecting the re-usable particle filtering half mask shall satisfy the penetration requirement of the relevant class.	Not applicable (Not designed to be re-usable)	N.A.

Clause 7.7 Practical Performance

(EN 149:2001+A1:2009, Clause 8.4)

Test Requirement	Results	Comment
The particle filtering half mask shall undergo practical performance tests under realistic conditions. These general tests serve the purpose of checking the equipment for imperfections that cannot be determined by the tests described elsewhere in this standard.	No imperfections	Pass



Clause 7.8 Finish of Parts

(EN 149:2001+A1:2009, Clause 8.2)

Test Requirement	Results	Comment
Parts of the device likely to come into contact with the wearer shall have no sharp edges or burrs.	No sharp edges or burrs	Pass

Clause 7.9.1 Total Inward Leakage

(EN 149:2001+A1:2009, Clause 8.5)

Test Requirement	Results	Comment
The total inward leakage consists of three components: face seal leakage, exhalation value leakage(if exhalation value fitted) and filter penetration. For particle filtering half masks fitted in accordance with the manufacturer's information, at least 46 out of the 50 individual exercise results (i.e. 10 subjects x 5 exercises) for total inward leakage shall be not greater than: 25% for FFP1, 11% for FFP2, 5% for FFP3 and, in addition, at least 8 out of the 10 individual wearer arithmetic means for the total inward leakage shall be not greater than: 22% for FFP1, 8% for FFP2, 2% for FFP3	Detail refer to Appendix 1	Meet FFP1 Meet FFP2

Appendix 1: Summarization of Test Data

Inward Leakage Test Data

Subject	Sample No.	Condition	Walk(%)	Head Side/side(%)	Head up/down(%)	Talk(%)	Walk(%)	Mean(%)
Zhou	1	A.R.	5.48	5.12	5.02	5.21	5.02	5.17
Luo	2	A.R.	6.72	5.73	5.18	7.34	5.08	6.01
Lu	3	A.R.	3.71	6.32	5.43	5.83	6.95	5.65
Wang	4	A.R.	4.43	4.87	5.15	4.04	4.11	4.52
Bao	5	A.R.	6.24	6.28	6.26	6.90	6.12	6.34
Ding	6	T.C.	5.11	4.23	4.29	4.89	4.80	4.66
Li	7	T.C.	5.99	6.89	5.02	6.64	7.48	6.40
Chen	8	T.C.	5.41	4.51	5.45	5.07	4.41	4.97
Song	9	T.C.	5.37	6.54	5.18	6.17	5.70	5.79
Ye	10	T.C.	7.48	6.86	6.08	6.60	6.80	6.76

Facial Dimension(mm)

Subject	Face length	Face Width	Face Depth	Mouth Width
Chen	125	150	120	58
Lu	115	132	107	48
Zhou	115	135	106	52
Li	125	130	107	46
Luo	125	136	100	43
Zheng	128	140	112	55
Wang	120	147	103	48
Song	120	140	100	50
Bao	130	134	104	50
Ding	134	150	110	52

Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com



Liu	120	135	117	50
Ye	126	137	105	52

Clause 7.9.2 Penetration of Filter Mater7ial

(EN 149:2001+A1:2009, Clause 8.11 & EN 13274-7:2019)

Test Requirement			Results	Comment
The penetration of the filter of the particle filtering half mask shall meet the requirements of the following table.			Detail refer to Appendix 2	Meet FFP1 Meet FFP2
Classifica tion	Maximum penetration of test aerosol			
	Sodium chloride test 95 l/min % max.	Paraffin oil test 95 l/min % max.		
FFP1	20	20		
FFP2	6	6		
FFP3	1	1		

Appendix 2: Summarization of Test Data

Penetration of filter material

Aerosol	Condition	Sample No.	Penetration (%)
Sodium chloride test	As received	1	1.472
		2	1.362
		3	1.472
	Simulated wearing treatment	4	1.386
		5	1.267
		6	1.347
	Mechanical strength + Temperature conditioned	7	2.067
		8	2.134
		9	2.124
Paraffin oil test	As received	10	2.544
		11	2.776
		12	2.813
	Simulated wearing treatment	13	2.708
		14	2.736
		15	2.748
	Mechanical strength + Temperature conditioned	16	3.542
		17	3.686
		18	3.281

Flow conditioning : Single filter: 95.0 L/min



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Clause 7.10 Compatibility with Skin

(EN 149:2001+A1:2009, Clause 8.4 & 8.5)

Test Requirement	Results	Comment
Materials that may come into contact with the wearer's skin shall not be known to be likely to cause irritation or any other adverse effect to health.	No irritation or any other adverse effect to health	Pass

Clause 7.11 Flammability

(EN 149:2001+A1:2009, Clause 8.6)

Test Requirement	Results	Comment
The material used shall not present a danger for the wearer and shall not be of highly flammable nature When tested, the particle filtering half mask shall not burn or not to continue to burn for more than 5 s after removal from the flame.	Detail refer to Appendix 3	Pass

Appendix 3: Summarization of Test Data

Flammability

Condition	Sample No.	Result
As received	1	NIL
	2	NIL
Temperature conditioned	3	NIL
	4	NIL

Clause 7.12 Carbon Dioxide Content of The Inhalation Air

(EN 149:2001+A1:2009, Clause 8.7)

Test Requirement	Results	Comment
The carbon dioxide content of the inhalation air (dead space) shall not exceed an average of 1,0 % (by volume)	Detail refer to Appendix 4	Pass

Appendix 4: Summarization of Test Data

Carbon Dioxide Content of The Inhalation Air

Condition	Sample No.	Result(%)
As received	1	0.4641
	2	0.4646
	3	0.4639
		Mean value:0.46



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgs.com.cn
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Clause 7.13 Head Harness

(EN 149:2001+A1:2009, Clause 8.4 & 8.5)

Test Requirement	Results	Comment
The head harness shall be designed so that the particle filtering half mask can be donned and removed easily.	Comply	Pass
The head harness shall be adjustable or self-adjusting and shall be sufficiently robust to hold the particle filtering half mask firmly in position and be capable of maintaining total inward leakage requirements for the device.	Comply	

Clause 7.14 Field of Vision

(EN 149:2001+A1:2009, Clause 8.4)

Test Requirement	Results	Comment
The field of vision is acceptable if determined so in practical performance tests.	Comply	Pass

Clause 7.15 Exhalation Valve(s)

(EN 149:2001+A1:2009, Clause 8.2 & 8.9.1 & 8.3.4 & 8.8)

Test Requirement	Results	Comment
(a) A particle filtering half mask may have one or more exhalation valve(s), which shall function correctly in all orientations.	Not applicable due to No exhalation valve	N.A.
(b) If an exhalation valve is provided it shall be protected against or be resistant to dirt and mechanical damage and may be shrouded or may include any other device that may be necessary for the particle filtering half mask to comply with 7.9.	Not applicable due to No exhalation valve	
(c) Exhalation valve(s), if fitted, shall continue to operate correctly after a continuous exhalation flow of 300 l/min over a period of 30 s.	Not applicable due to No exhalation valve	
(d) When the exhalation valve housing is attached to the faceblank, it shall withstand axially a tensile force of 10N applied for 10 s.	Not applicable due to No exhalation valve	



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgs.com.cn
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Clause 7.16 Breathing Resistance

(EN 149:2001+A1:2009, Clause 8.9)

Test Requirement				Results	Comment
The penetration of the filter of the particle filtering half mask shall meet the requirements of the following table.				Detail refer to Appendix 5	Meet FFP1, Meet FFP2, Meet FFP3
Classification	Maximum permitted resistance (mbar)				
	Inhalation		Exhalation		
	30 l/min	95 l/min	160 l/min		
FFP1	0.6	2.1	3.0		
FFP2	0.7	2.4	3.0		
FFP3	1.0	3.0	3.0		

Appendix 5: Summarization of Test Data

Breathing resistance (mbar)

	Flow rate(l/min)	1					2					3					
		A	B	C	D	E	A	B	C	D	E	A	B	C	D	E	
As received	Inhalation	30	0.4	0.4	0.5	0.3	0.4	0.5	0.3	0.5	0.3	0.3	0.4	0.5	0.4	0.3	0.4
		95	1.5	1.6	1.5	1.5	1.6	1.5	1.6	1.5	1.6	1.5	1.5	1.5	1.6	1.5	1.5
	Exhalation	160	2.0	2.1	2.0	2.0	2.1	2.0	2.1	2.0	2.1	2.1	2.1	2.0	2.1	2.0	2.1
Simulated wearing treatment	Inhalation	30	0.4	0.4	0.5	0.3	0.4	0.5	0.4	0.5	0.3	0.4	0.5	0.4	0.3	0.5	0.4
		95	1.5	1.6	1.6	1.5	1.6	1.5	1.6	1.6	1.5	1.6	1.5	1.6	1.6	1.5	1.6
	Exhalation	160	2.1	2.2	2.1	2.1	2.2	2.1	2.2	2.1	2.2	2.1	2.1	2.2	2.1	2.2	2.1
Temperature conditioned	Inhalation	30	0.3	0.4	0.4	0.3	0.4	0.3	0.3	0.4	0.3	0.4	0.4	0.3	0.4	0.3	0.4
		95	1.4	1.5	1.5	1.4	1.5	1.4	1.5	1.4	1.4	1.5	1.4	1.5	1.4	1.5	1.4
	Exhalation	160	2.1	2.2	2.1	2.1	2.2	2.1	2.1	2.2	2.1	2.1	2.1	2.2	2.2	2.1	2.1

A: facing directly ahead; B: facing vertically upwards; C: facing vertically downwards; D: lying on the left side; E: lying on the right side



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.
Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
 SGS-CSTC Standards Technical Services (Shanghai) Co., Ltd. 3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
 Testing Center: No.889, Yishan Road, Xuhui District Shanghai, China 200233 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Clause 7.17 Clogging

(EN 149:2001+A1:2009, Clause 8.9 & 8.10)

Test Requirement	Results	Comment																			
<p><u>Clause 7.17.2 Breathing resistance</u> <u>Valved particle filtering half masks:</u> After clogging the inhalation resistances shall not exceed: FFP1: 4 mbar, FFP2: 5 mbar, FFP3: 7 mbar at 95L/min continuous flow The exhalation resistance shall not exceed 3 mbar at 160 L/min continuous flow.</p> <p><u>Valveless particle filtering half masks:</u> After clogging the inhalation and exhalation resistances shall not exceed: FFP1: 3 mbar, FFP2: 4 mbar, FFP3: 5 mbar at 95L/min continuous flow</p>	Optional for single shift device only	N.A.																			
<p><u>Clause 7.17.3 Penetration of filter material</u> All types (valved and valveless) of particle filtering half masks claimed to meet the clogging requirement shall also meet the requirements.</p> <table border="1"> <thead> <tr> <th rowspan="3">Classification</th> <th colspan="2">Maximum penetration of test aerosol</th> </tr> <tr> <th>Sodium chloride test 95 l/min</th> <th>Paraffin oil test 95 l/min</th> </tr> <tr> <th>%</th> <th>%</th> </tr> </thead> <tbody> <tr> <td></td> <td>max.</td> <td>max.</td> </tr> <tr> <td>FFP1</td> <td>20</td> <td>20</td> </tr> <tr> <td>FFP2</td> <td>6</td> <td>6</td> </tr> <tr> <td>FFP3</td> <td>1</td> <td>1</td> </tr> </tbody> </table>	Classification	Maximum penetration of test aerosol		Sodium chloride test 95 l/min	Paraffin oil test 95 l/min	%	%		max.	max.	FFP1	20	20	FFP2	6	6	FFP3	1	1	Optional for single shift device only	N.A.
Classification		Maximum penetration of test aerosol																			
		Sodium chloride test 95 l/min	Paraffin oil test 95 l/min																		
	%	%																			
	max.	max.																			
FFP1	20	20																			
FFP2	6	6																			
FFP3	1	1																			

Clause 7.18 Demountable Parts

(EN 149:2001+A1:2009, Clause 8.2)

Test Requirement	Results	Comment
All demountable parts (if fitted) shall be readily connected and secured, where possible by hand	No demountable parts	N.A.

Test	Uncertainty
Total inward leakage	3.4%
Penetration of filter material	4.8%
Carbon dioxide content of the inhalation air	3.9%
Breathing resistance (30L/min)	5.9%
Breathing resistance (95L/min)	4.9%
Breathing resistance (160L/min)	4.3%




Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing / inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com

SGS-CTC Standards Technical Services (Shanghai) Co., Ltd. 3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
 中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com

Sample Photo

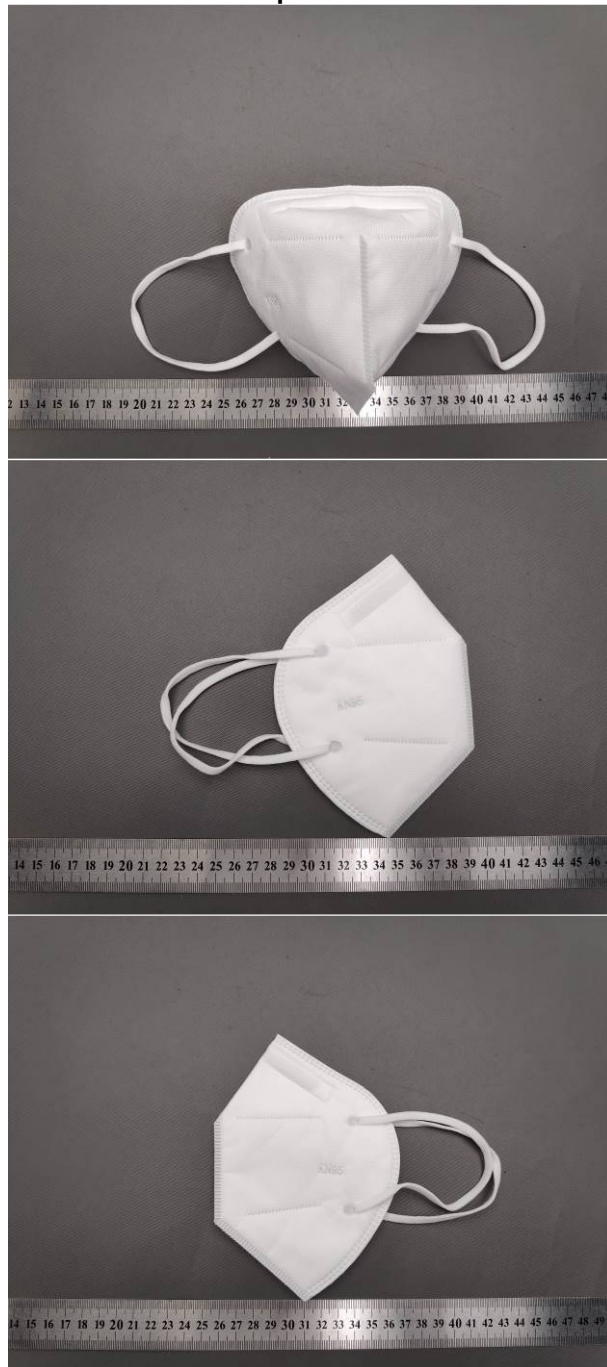

End of Report



Unless otherwise agreed in writing, this document is issued by the Company subject to its General Conditions of Service printed overleaf, available on request or accessible at <http://www.sgs.com/en/Terms-and-Conditions.aspx> and, for electronic format documents, subject to Terms and Conditions for Electronic Documents at <http://www.sgs.com/en/Terms-and-Conditions/Terms-e-Documents.aspx>. Attention is drawn to the limitation of liability, indemnification and jurisdiction issues defined therein. Any holder of this document is advised that information contained hereon reflects the Company's findings at the time of its intervention only and within the limits of Client's instructions, if any. The Company's sole responsibility is to its Client and this document does not exonerate parties to a transaction from exercising all their rights and obligations under the transaction documents. This document cannot be reproduced except in full, without prior written approval of the Company. Any unauthorized alteration, forgery or falsification of the content or appearance of this document is unlawful and offenders may be prosecuted to the fullest extent of the law. Unless otherwise stated the results shown in this test report refer only to the sample(s) tested and such sample(s) are retained for 30 days only.

Attention: To check the authenticity of testing /inspection report & certificate, please contact us at telephone: (86-755) 8307 1443, or email: CN.Doccheck@sgs.com
3rd Building, No.889, Yishan Road, Xuhui District Shanghai, China 200233 t (86-21) 61402666 f (86-21) 64958763 www.sgsgroup.com.cn
中国·上海·徐汇区宜山路889号3号楼 邮编: 200233 t (86-21) 61402666 f (86-21) 64958763 e sgs.china@sgs.com